


## Information from Data File:

File :D:\RMP\12-501 ITEM 1.D  
Operator : RMP  
Acquired : 27 Mar 2012 12:13 using AcqMethod LOWBOIL.M  
Sample Name: Proficiency Test  
Misc Info : 12-501 ITEM 1  
Vial Number: 3  
Instrument : HP5975

Search Libraries: C:\Database\LIBA.L Minimum Quality: 90  
C:\Database\LIBT.L Minimum Quality: 80  
C:\Database\NIST08.L

Unknown Spectrum: Apex  
Integration Params: rteint.p

Pk#	RT	Area%	Library/ID	Ref#	CAS#	Qual
1	2.38	78.97	C:\Database\NIST08.L Dimethyl sulfone	2507	000067-71-0	83

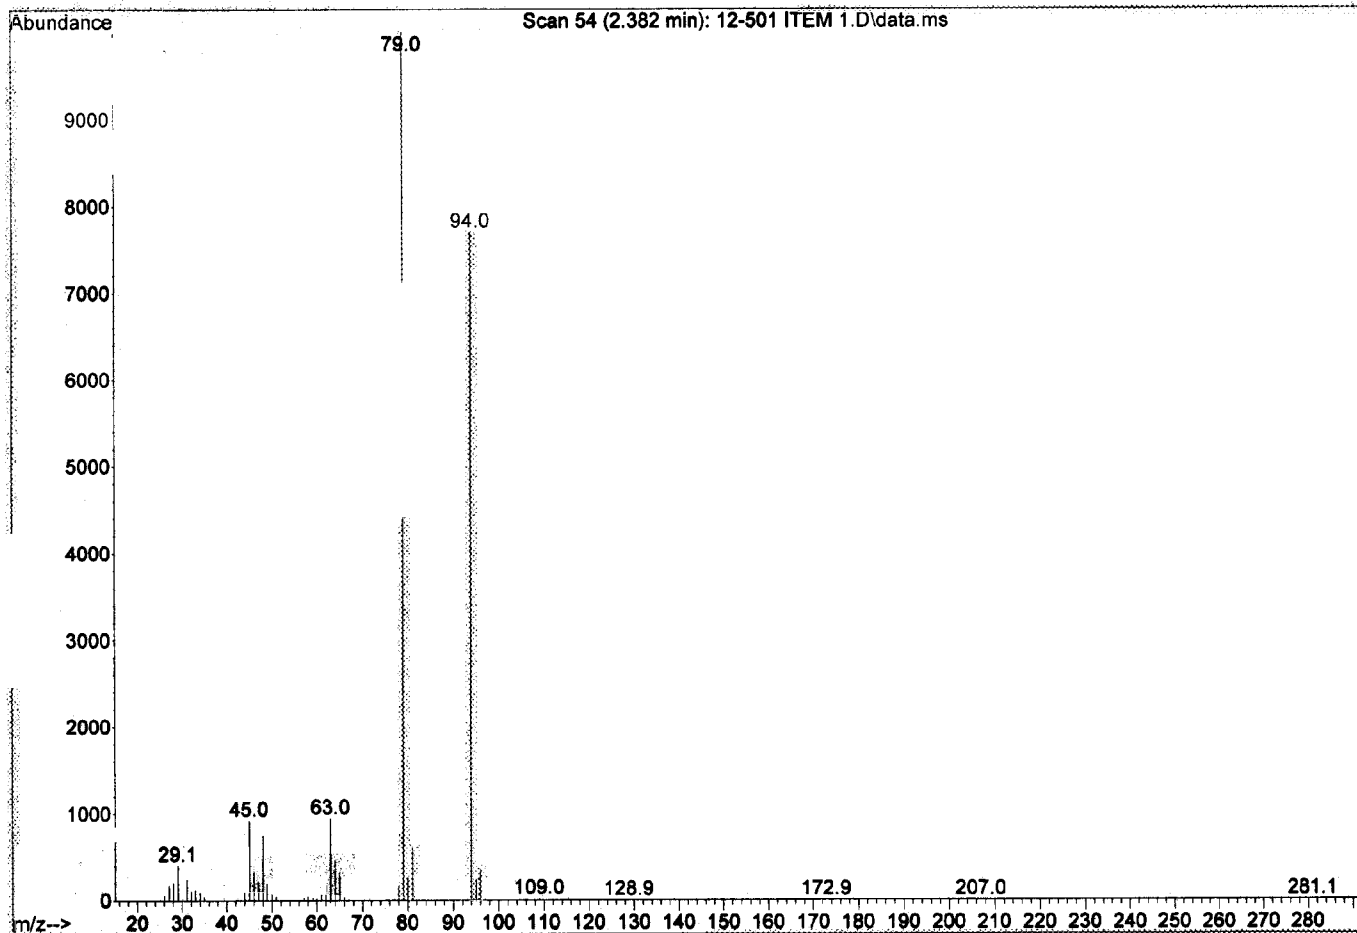

M/Z	Abundance
27.10	175
28.10	197
29.10	402
31.10	244
32.00	105
33.00	119
45.00	917
46.00	333

M/Z	Abundance
47.00	206
48.00	747
49.00	190
62.00	191
63.00	942
64.00	466
65.00	280
78.00	162

M/Z	Abundance
79.00	10000
80.00	263
81.00	596
94.00	7699
95.00	249
96.00	347